

References

1. Baek SH. Identification and preoperative optimization of risk factors to prevent periprosthetic joint infection. *World J Orthop* 2014;5(3):362-367
2. Kurtz SM, Lau E, Watson H, Schmier JK, Parvizi J. Economic Burden of Periprosthetic Joint Infection in the United States. *J Arthroplasty* 2012;27(8), Suppl 1:61-65.e1
3. Gundtoft PH, Overgaard S, Schonheyder HC, Moller JK, Kjaersgaard-Andersen P, Pedersen AB. The "true" incidence of surgically treated deep prosthetic joint infection after 32,896 primary total hip arthroplasties. A prospective cohort study. *Acta Orthopaedica* 2015; 86(3):326-34
4. Trampuz A, Maiolo EM, Winkler T, Perka C. Biofilm formation on ceramic, metal and polyethylene bearing components from hip joint replacement systems. Abstract ISTA 2015
5. Beraudi A, Stea S, Pasquale D, Bordini B, Catalani S, Apostoli P, Toni A. Metal ion release: also a concern for ceramic-on-ceramic couplings? *Hip Int* 2014;24 (4): 321-326
6. Esposito C, Maclean F, Campbell P, Walter WL, Walter WK, Bonar SF. Periprosthetic Tissues From Third Generation Alumina-on-Alumina Total Hip Arthroplasties. *J Arthroplasty* 2013;28:860-6
7. Streicher RM, Porporati A. News on ceramics – beyond wear reduction. *Hip Int* 2014;24 (5):515
8. Bozic KJ, Ong K, Lau E, Kurtz SM, Vail P, Rubash H. Risk of Complication and Revision Total Hip Arthroplasty Among Medicare Patients with Different Bearing Surfaces. *CORR* 2010;468;2357-2362
9. Trebse R, Levasic V, Kovac S. Prosthetic Joint Infections and bearings. *Hip International* 2014;24(5), 533
10. Aljaniipour P, Restrepo C, Smith L, Parvizi J, Malkani A. Periprosthetic joint infection: Could Bearing Surface Play a Role? Presentation 45th Annual Meeting Eastern Orthopaedic Association 2014
11. Smith L, Aljaniipour P, Restrepo C, Maltenfort M, Parvizi J, Malkani A. Periprosthetic joint infection: Could Bearing Surface play a Role? Abstract, 45th Meeting of the Eastern Orthopaedic Association 2014, 197
12. 12th Annual Report: National Joint Registry for England, Wales and Northern Ireland, 2015
13. Falcioni S, Ancarani C, Bordini B, Pichierri M, Stea S. Influence of articular coupling on septic loosening of total hip arthroplasty. Abstract EHS 2014
14. Varnum C, Pedersen AB, Kjaersgaard-Andersen P, Overgaard S. Comparison of the risk of revision in cementless total hip arthroplasty with ceramic-on-ceramic and metal-on-polyethylene bearings. *Acta Orthopaedica* 2015;86(3)
15. Graves SE, Lorimer M, Bragdon C, Muratoglu O, Malchau H. Reduced risk of revision for infection when a ceramic bearing surface is used. Abstract ISTA 2015
16. Pitto RP, Sedel L. Periprosthetic Joint Infection in Hip Arthroplasty: Is There an Association Between Infection and Bearing Surface Type? *Clin Orthop Relat Res* 2016; DOI 10.1007/s1999-016-4916-y


BIOLOX®*delta* ball heads and inserts, BIOLOX®OPTION as well as the knee implants made of BIOLOX®*delta* are registered by CeramTec's customers. They are not registered / available in all countries. The shoulder implants made of BIOLOX®*delta* are under development and are not approved by any authorities.

CeramTec
THE CERAMIC EXPERTS

BIOLOX® is a registered trademark.
© 2017 CeramTec GmbH www.biolox.com



BIOLOX[®] inside
Beyond comparison since 1974

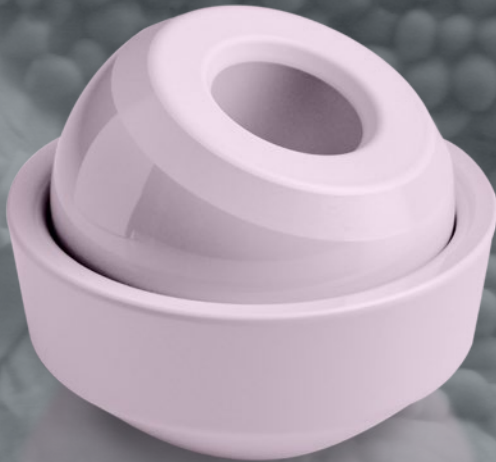

BIOLOX[®] *delta*
Ceramics Reduce
the Risk for PJI
Revisions in THA

CeramTec
THE CERAMIC EXPERTS

Periprosthetic Joint Infection (PJI)

- PJI is the most devastating and costly complication of THA¹
- PJI is the third most frequent indication for revision in THA and its prevalence is on the rise²
- Up to 40% of revisions for aseptic loosening are undiagnosed PJI³



BIOLOX[®] inside
Beyond comparison since 1974

- BIOLOX[®] ceramics provoke only low biofilm adhesion⁴
- BIOLOX[®] *delta* is safe in terms of metal ion release⁵
- Soft-tissue inflammation may be clinically insignificant in THA with BIOLOX[®] ceramic bearings⁶



Registries show less revisions for PJI when BIOLOX[®] ceramic components are used⁷

